
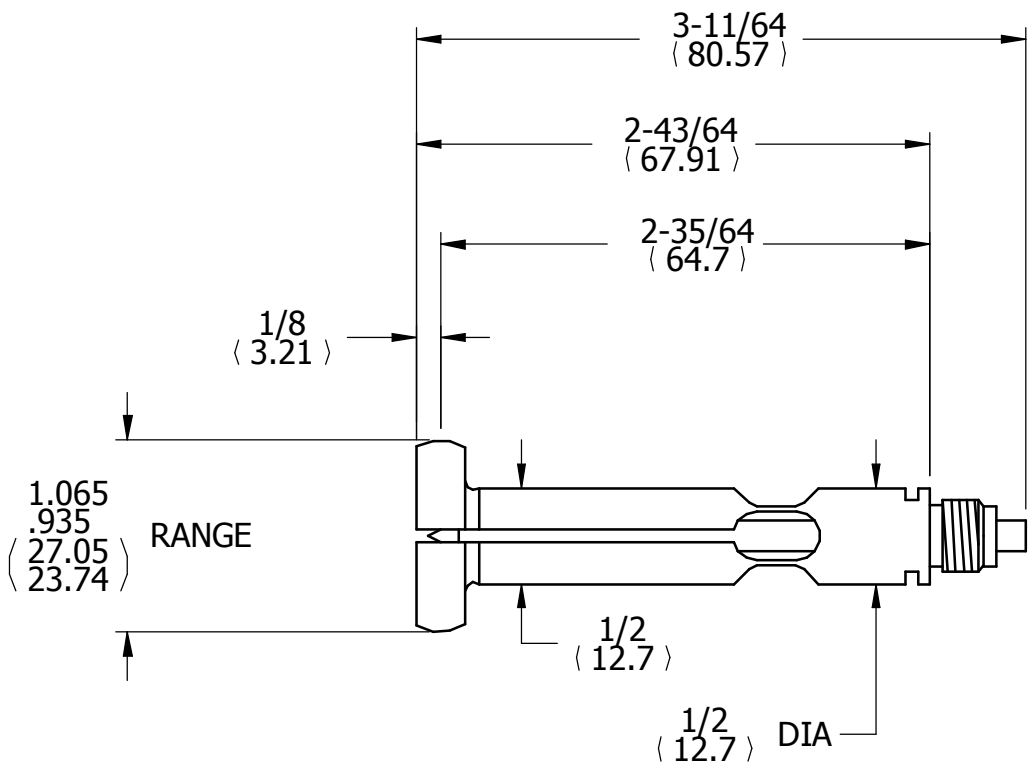


OPER

TOOLS



REV	DESCRIPTION	DATE	BY
DR	DSP	CHK	DATE
PROBE/ACTUATOR ASSEMBLY			
THE L.S. STARRETT CO. ATHOL, MASS.			

FRACTIONAL TOLERANCE +- 1/64 UNLESS OTHERWISE NOTED